

A Standardised Review On Ankle-Foot Exoskeleton

G.Gowrishankar¹, A Arockia Selvakumar²

*Research scholar, School of Mechanical Engineering, Vellore Institute of Technology, (Deemed to be University), Chennai, Tamilnadu, India,
Email:gowri.shankarg2014phd1121@vit.ac.in*
*Senior Associate Professor, of Mechanical Engineering, Vellore Institute of Technology, (Deemed to be University), Chennai, Tamilnadu, India,
E mail:arockia.selvakumar@vit.ac.in*

Corresponding Author:

*Dr.A.Arockia Selvakumar, Senior Associate Professor, of Mechanical Engineering, Vellore Institute of Technology, (Deemed to be University), Chennai, Tamilnadu, India,
E mail:arockia.selvakumar@vit.ac.in*

ABSTRACT

Objective: *The objective of this article is to review the gait analysis of various ankle-foot exoskeletons by different techniques.*

Overview: *Gait exploration, the methodical learning of striding, is a domain that has been deliberated over 90 years. With automation and research-based improvements over the previous decade, there has been significant enhancement in our perception of the mechanics of strolling of human. Especially salient features have been the development in discrimination of the dissimilarity among standard and morbid gait.*

Conclusion: *This may assist Ankle –foot Exoskeleton also Orthopedics physician in superior perception, the procedures and synonym of gait perceive the proclamations that generally materialize in the Ankle –foot Exoskeleton also ankle operation compositions.*

Summary: *An intention of this paper is to appraise the postulates of gait investigation, with a certain focal point on the fundamental techniques and field science. A systematic appraise of ankle-foot striding experience have been gathered and furnished a summary for future works.*

Keywords: *Gait exploration, Biomechanics, Morbid gait, Orthopedics physician .*

INTRODUCTION

An ankle-foot orthosis is an assist considered to manage the fixture and movements of the ankle and remunerate condition. Analysis of human gait is the theme of numerous assess, which provides valid information about the development of diseases like stroke, Parkinson etc. The ankle joint takes a vital part in gait basis. The effective function of gait like load adoption, bearing on a single limb, and enhancement of limb are based on the actual operation of the ankle joint. Ankle -foot mechanics have made a crucial enhancement over the previous decades with fundamental variety of outcomes for gait analysis and rehabilitation. The methodological appliances used to find striding on ankle-foot can be done in two strategies: wearable sensors (WS) and non-wearable sensors (NWS).WS model is employed with sensors over the body to acquire input data via each action of individuals through gait. In contrast, NWS model use the manageable investigation potentials, which are placed in a fixed location and gain input on gait. In this review, we employ wearable sensor structure to assess ankle-foot gait analysis using the exoskeleton shown in Figure 1.



Figure 1: Existing exoskeleton model for Ankle-Foot Orthosis (Yufeng Zhang et al. [1])

The above illustration is used to control and manage the design for exoskeleton by reducing undesired interaction without any extra sensors in the process of ankle-foot orthosis. Objective of this method review was to estimate and summarize the perusal of gait. The following surveys are made to collect information about existing wearable exoskeleton model. AFO wearable model are heavy in weight, have increased the burden on the limbs of stroke survivors. Therefore, more study has to be done to change the pattern of gait to reduce the weight of the wearable model. High torque output actuators may be further developed to reduce the burden of the lower limb in wearable models. As the study of the gait detection of post stroke population is not properly supported, the detection can be improved by considering the people's pattern of walking. Research based on inversion and eversion assistance in wearable model design can be done further to improve the muscle strength and promote the gait rehabilitation, because existing wearable AFO model assists only dorsiflexion and plantar flexion. Present model of wearable AFO do not support application based trials like treadmill and over ground training in stroke patients. So, in order to achieve maximum efficiency in medical application, large samples in random manner over many centres under clinical control should be done. The study of this work is done to diagnosis using image processing technique to find at what extent the damage is seen in ankle foot and so that the treatment of ankle foot orthosis can done with perfect design of exoskeleton model or it could even treated by surgery. It is essential to initiate the present evince basis to realize what corroboration subsist further what supplemental investigation is required. This literature study demonstrates practical, prognosis exactness of gait perusal on ankle-foot by adopting exoskeleton.

Bio-Mechanical Analysis Of Gait By Different Trajectories

Documentary research was regulated to recognize references associated with ankle-foot perusal issued between 2015 and 2020, also with additional research studies. We bounded to explore towards Bio-Mechanical analysis of gait using different quantitative methods ie; wearable sensors, non-wearable sensors and image processing as these hold the majority of the reviews on ankle-foot perusal. In case of wearable sensors AFO model, there exist two types of wearable exoskeleton model they are: soft wearable exoskeleton and rigid wearable exoskeleton. Wearable system has many advantages in real time and restrictions in laboratory. For instance in real time applications, gait analysis can be done and monitored for long duration of time but in lab testing it allows assessment for few number of gait specifications. Major advantages of wearable AFO are, they have no restriction in controlled surroundings, movable and cost efficient. Few wearable sensors like goniometers, accelerometers etc., are used to develop a wearable AFO to overcome the drawbacks of conventional system. The basic concept of wearable exoskeleton model is to track the movements of the patient and do the analysis on gait using the sensors. In

order to analyze the motion of the patient's body, the sensors are fixed to respective sections of the body and the tracking of the motion is done. For example, inertial sensor is one among the wearable sensors being used. The purpose of this sensor is to track the orientation and position of the human body.

Gait Analysis Of Ankle Foot Orthosis Using Sensors

On the basis of adaptable frequency controllers, Zhang et al.¹ propounded an advance transparent controller. Appraisal alterations proved that, it can crucially upgrade technique transparency collated to a conventional controller. An advanced controller can notably upgrade the purity of the system. Also, this system is robust to variations in walking speed and achieve smoothly the brace in completely-energetic and in partially-energetic actuation methods.¹ To identify the shortage of an appraisal and to make a treatment efficiently, Bolus et al.² introduced an Intermittent Ankle-Foot Orthosis (IAFO) that can be utilized to measure an effective outcome of particularly altering the ankle joint hardness. It has been developed to recognize and appraise certain shortfalls. It is competent of brace appealing orthotic resistance as well as observing a substantial set of appropriate objective parameters recurrently and authentically, so Sanz-Morere et al.³ developed an appliance that could be practicable make out while hidden beneath classic usual attire, featuring the stimulating prospective for the extensive acquisition of gait methods towards the community would be for the sake of wider extent of solitary. Each wearable mechanisms will possess with diverse features, among these prospects, Ding et al.⁴ offered a biomechanical and objective assessment and collected the consequences of furnishing assistance with a spongy assisting device to any one of a single or multiple joints which upgrade walking efficiently throughout freighted. To diminish the procedure utilization price, as well as to deploy in a soft manner this kind of exoskeleton has been developed associated with fixtures aspect to the body. The previous braces strategies enable for flexibility and comfort of assisting devices for the sufferer. Akhil et al.⁵ examined the gaits on humans, with the assistance of lofty intention camera for fit and related the theme on the base level. It offered an appropriate managing system to provide a fine firmness. It considers only the appraisal for usual striding.

To overcome the demerits of above discussed method Rachel W. Jackson and Steven H. Collins⁶ proposed an appraisal for helping mobility with assisting devices. It will be complicated to predict the alterations via painless walking procedures with muscles that presume the fastened motion. Particulars from this appraisal can be employed to anticipate the contractile organ changing further direct to the scheme of aid appliances. Chen et al.⁷ evolved an adaptable oscillator to evaluate the footstep of the assisting device connection on the exoskeleton activities. This process proposes the harmonization with unusual gait models and the execution towards recovery robots were viable. This was further developed by Sanz-Morere et al.³ redesigned a KAFO base phase manage model further revealed sufficient execution. It has been collated with remaining robotic gaits and provided an efficient gait stage. It connections on torque with movements are associated action. A complex pendulum system has been pertained to analyse the oscillations stage of movement for the exoskeleton of the lower limb as well as the ankle-foot was proposed by Miao et al.⁸ The resonant interval of ankle-foot can be diminished by elevating the angle in a striding phase of several frequencies. So, Sanchez-Villamanan et al.⁹ designed and collated the mechanical scheme possibilities of fifty lower limb exoskeletons grouped on features of complying like impetus, formation, boundary, fitment constituents. But Zelik and Honert¹⁰ explained about abandon of ankle feet can obstruct the scientific comprehension of motion; astonish our potential to make robust clinical examination.

To overwhelm these complications, Chen et al.¹¹ designed a transferrable gait analysis of ankle, knee for stroke sufferer on basis of biomechanical wearable sensor. The objective is to anticipate the gait deficit and the irregular stages which are determined via HMM. Also Zhao et al.¹² evaluated artificial ankle-foot strength normally and deliberated the distortion velocity. DLS perusal was collated with UD as well as DF process further grants the formation of distortion of artificial ankle-foot constituents individually. While, Novak and Riener¹³ offered sensor combination investigation in wearable robotics are inter-modal, versatility and appraisal

assessment. Virtually, it is vital to concern on multimodal sensor combination and secures benefits of flexible categorizer also shifting and blending techniques. Rather than other surveillance, the following research reveals neither sensors nor mechanical attachments are fixed with it. In order to overwhelm this, Wang et al.¹⁴ illustrated a shrewd clutch, which is meld with a sensor-controller that includes braces penetrating and implementing part. Supremacy involved in this technique reveals that the clutch is insubstantial and dependable. Also, the anticipation of gait reckons on the available separating foot and floor, therefore the clutch is universal and dispensable to personalize. In connecting with other researchers it associated a further advancement such as resistors and persistent alarm to diagnose deficits in an appraisal. So, Yu et al.¹⁵ utilized this statistical thesis which comprised of sliding window detector as well as a constant false alarm rate (CFAR) procedure to determine the gait influence in recent model. Already mentioned detector split up GCF (ground contact force) into 3 zones. Eventually, gait influence could be esteemed connection on the perception directives and gain lofty dependability. Independent exoskeletons also have been fitted based on the measurement of torque by utilizing and progress by the data examined by Mooney and Herr.¹⁶ It indicates a dynamic free ankle assisting device which is a biomechanical process utilized for incorporate depletion. It does not diminish the mechanical power at the ankle however also diminished in the knee and hip, as collated to movement lacking exoskeleton. It is feasible to provide high metabolic depletions.

Taborri et al.¹⁷ recognized, chose, group the obtainable techniques for gait stage perception, scanning supremacy and pitfall of individuals. Eventually, investigate the available gait stage coarseness, practicable techniques and ideal sensor positioning on the body parts. Likewise the same, the threshold strategy via FSR can be noted by locomotion in a real-time by Tang et al.¹⁸ tendered an STTA (self-tuning triple-threshold) process that estimates gait levels in recent and reveals flexibility to discern mobility constraints. It attains a steady fidelity in 5 appraisals with the dissimilar walking speed at knowing times. Long et al.¹⁹ offered standard type is effective and reasonable for the LEE (lower extremity exoskeleton). Along with biomechanical and sensor attachments, this appliance has been evolved. Collected with previous techniques and furnished few aspects like feasible pHRI mensuration appliance to heed mobility, the associated controller model has been designed to make a gait thin and solid. Farah et al.²⁰ offered a planning model decision in three categorizer. The study for several imitated striding circumstances accomplished over everyday activities was made. This perusal proved that AI can furnish upgraded gait stage realization. Choi et al.²¹ estimated the process of AFO rigidity effects kinematics as well as MG basis through damaged gait. AFO possesses a lofty rigidity also its peak got elevated. Similarly, this process has diminished. Arnez-Paniagua et al.²² proposed a flexible controller for AAFO. The depletion of TA as well as GA muscular functions demonstrated the effectiveness of the offered model to aid gait of foot-drop concepts. In associations with an objective control procedure, could possess the capability to be enacted with foot-drop victims for normal subsistence actions to diminish the motility of the sufferer fluctuating.

For assisting device in robotic management for continuous striding aid in reputation of real-time, so an advanced technology has been established by Fataisado et al.²³ he pondered an exoskeleton handle method for simultaneous striding aid in managing activities that include long hours of striding. The appraisal alterations revealed that this model could be implemented to well-being labourer where motion habitat may be irregular and complex. Later a model was developed with precise lubrication of SFS (Selective Laser Sintering) along with CAD mechanism, an appliance has been designed by Faustini et al.²⁴ Connect the CF-AFO towards PD-AFO production of mechanical dampened via SLS which manifest the slightest amount of strength decadence and was the solitary stuff to resist destructive assess. Oba et al.²⁵ offered an evolvment of a linear elastic joint and MR fluid. The upgraded APO furnished manageable braking in prior. The combination of passive constituents as well as fine stuff can generate the link for a feasible and effective aid method. Brown et al.²⁶ scanned the consequences of AFO arrangement on lower limb mechanics also solitary involved muscle movements. The Alterations declared that the compact ($< 5^\circ$) variation in AFO possesses a vital consequence on ankle and knee joint activities.

French et al.²⁷ suggested that exactness of kinetics GED strategies in stroke victims is a process of upgrading the standard of gait investigation separately with gait diversions. Eckardt and Kibele²⁸ exhibited the efficient application procedure on basis of kinetics for gait perception on irregular surfaces with dissimilar speed. An external arrangement also pace of striding possess a cause on exactness, however compact dimensions are also the persistent of regulation inconsistency.

Castellanos et al.²⁹ utilize AFFO for a typical tracking process in recovery's sake. An intention of the appraisal is to estimate the feasibility of the model to aid the gait of a good specialism. The effectiveness of the ADRC archetype is authenticated the conceptual investigation. Hyun et al.³⁰ proposed a HUMA which is a biomedical model for the lower limb exoskeleton. Specifically, an active running gait declares, that the proficiency of the robotic leg associated accurately with the human leg, which reveals capability for the proposed scheme in further exoskeletal implementations.

Later, Pardoel and Doumit³¹ pondered a passive WAE that gathered strength from posture shift of gait to furnish aid at the push-off stage. The kinetics of appliances was imitated link on the gait data of an independent. Thus the firmness of PAM causes an extent of motion also the range of aid furnished through the exoskeleton. So equality attains an efficient upshot. Sherwani et al.³² designed a RISE administrator to attain optimal tracking inconsistency which has been blend with related concepts to remunerate the cause for irregular interruptions. The controller furnishes the appropriate production namely tracking inconsistency while exposed to disruptions occurred. Yandell et al.³³ proposed a lightweight, low-cost unpowered ankle exoskeleton, suitable for various walking speeds without restricting joint motion with usable ankle torque that may reduce demands on the biological calf musculature. The design integrates a low profile under-the-foot clutch and a soft shank interface, joined by an ankle aid spring that operates in parallel with the user's calf muscles it can be used on a wide scale to benefit a broad range of individuals throughout society, such as the elderly, individuals with impaired plantar flexor muscle strength, or recreational users. Overall study of AFO using sensors were made, this analysis is the integration of control techniques. Every control techniques has its own controllers, each controller has its own advantages and drawbacks. Different controllers were implemented on the same hardware design, made the study difficult. The main aim of the analysis is to provide maximum comfort to the human having ankle foot orthoses, though many developments were made in the controller design still changes should be done to increase the efficiency and the effectiveness of the design. The proper control technique can provide a safe and comfortable human computer interaction in gait training, trigger patients' eagerness for rehabilitation, and thus improve the effect of gait rehabilitation.

Gait Analysis Of Ankle Foot Orthosis By Image Processing

This algorithm utilizes digital image processing strategies to lay a simpler process of ankle-foot of gait analysis. The distinctive IP model is structured via various digital PCs that can be utilized to collect relevant gait particulars. PO aids to detect the movements of ankle-foot via gait analysis. This perusal can be segmented and classified. An image processing technique has been introduced here to acquire precise particulars by processing cycles of motion in a computerized or autonomous manner. Agostini et al.³⁴ offered a prevalent basis procedure for the categorization of gait cycles. It has been utilized for clinical investigation of gaits also granted the establishment of unusual cycles offers in sufferer locomotion. The ankle-foot prints have been segmented and the prospects to estimate the percent of the contingency of different cycles of movement. This procedure is the preliminary stage of processing a statistical perusal of movement, yet it furnishes the demand categorization. Using an adaptive classification, the procedure has been scrutinized the viability of appealing an adaptable categorization type for upgrading model dependability when input gestures changes developed. Besides, the adaptable transferring state identification procedures gain dependable assisting devices across scrutinizing periods. The neuro-muscular mechanism based on the LMR procedure combination, the process has been carried out by Liu et al.³⁵ Simulated strength of the fluctuations scheme has been established.

HousseinLamine et al.³⁶ proposed a CDLT model which is connected on movement seize system and therefore progression of gait rehabilitation can be evaluated. The outcome of the investigation was utilized to ascertain the vital strength of the controllers. Recently, Abe et al.³⁷ pondered the EEFJ (elastomer-embedded flexible joint) model and fixed a braces EEFJ on handcrafted ankle orthopedic appliance. It diminished the load on the tibialis antecedent muscle in the prior posture and oscillates stages. However, the certain exercise of sufferers in perceptive robotic aid may possess a necessary influence on the outcome of locomotion, to overcome this drawback Tamburella et al.³⁸ introduced an appropriate robot called Achilles to aid the ankle while striding, was designed for ISCI (incomplete spinal cord injury) theme and employed the NMC (Neuromuscular Controller). Acquired upgrades and gait pace, so offered a capability recovery influence. The four linkage assisting device has been evolved. Roy et al.³⁹ made a study on the drawbacks and then he examined a disparity of pressure dispersion model beneath foot while mobility in 2004. The examination of the usual gait model and irregular gait model because of dissimilar persistent constraints could be examined. Moreover via the EMG investigation of muscles while rolling a relation separating muscular action along with pressure dispersion beneath the foot for usual and irregular gait can be evolved. Singh et al.⁴⁰ developed a gait grounded composite process which evolves submerging in orthotic or exoskeleton, recovery appliances. It can be elongated by concerning complex linkages in the sector of firm links and manageable 4 bar links. The Alteration s of individual strategies are obtained also a two-level maximization level is secured to diminish the links and flaws further stimulate in MATLAB.

The gait realization method on basis of observing the movement fluctuates of body parts which were controlled via sensors by Davrondzhon Gafurov and Einar Snekkenes⁴¹. The study declare that loaded worn gaits inclined to lessen gaits intolerance also several sub-events accord dissimilarly in related to realization implementation. Least extremity was procured from MRI outcome further it has been connect with real-time locomotion gait experience based on a few aspects like dimensions, fixture etc. by utilizing the FE investigation model Nieto-Hidalgo et al.⁴² suggested a common gait identification of a procedure competent of impulsive extracting kinetics aspects. Initially capturing RGB illustrations further appealing procedures such as heel strike and toe-off (HSTOD), Fast Approximate Skeleton Extraction (FASE), K-Nearest Neighbors (KNN) then the production era is less collated to frame period. So, Park et al.⁴³ offered a biomechanical analysis of beneath ferocity in movement through FE investigation blend with mobility. It comprises of exterior active movements like GRF also interior dynamic force like muscle forces by focusing on coercion dispersion at the knee, ankle. But Yan et al.⁴⁴ proffered a voting-weighted integrated – Deep neural network is shown in Figure-2 (VWI-DNN) processes to examine multidimensional furthering fluctuates and determine various process like HS, FF, HO, SW. It delivers a lofty exactness. Moreover, the procedure utilized can yet attain a better realization of precise value, which is loftier of 98% accuracy. VWI-DNN scheme furnished a detailed forecast result also an enhanced gait perusal neglects the reputation inconsistency.

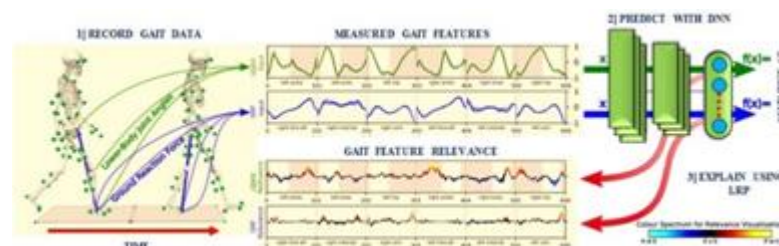


Figure 2: Pattern of Gait using Neural Network

To improve the result Nieto-Hidalgo et al.⁴⁵ proposed a feasible and effortless strategy to acquire HS, TO in braces sagittal as well as the frontal approaches. The capability to process gait

investigation via frontal side diminishes the physical interval needed for the examinations. Dynamic and usual gait to evaluate via cloud-based as well as individual activities have been recorded. In the case of leg-angle sequence data, it attained a cent percent accuracy further furnish a result by processing data, so Muro-de-la-Herran et al.⁴⁶ presented a common survey of individuals of gait analysis strategies. Eventually utilized methodologies like TUG also timed 25-foot. An idea is categorized as image processing sensors that have aspects that made them effective in various requirements. Because of this, Iaquinto et al.⁴⁷ designed a model connecting on tracking procedure which attentiveness towards the ankle and knee kinetics. Further authenticate the production of the biplane model of the tracking process allows a standard and finite motion. IRT (Infrared Thermography) has been employed to process an image to attain significant striding samples further by appealing KF filter obtained particulars and will enhance a rehabilitation procedure is shown in Figure 3.

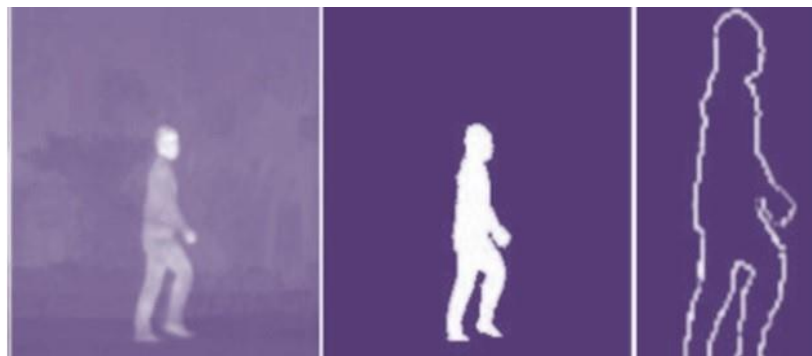


Figure 3: Processing on Image via striding analysis

So, Al-Qassab et al.⁴⁸ engrossed on the general non-traumatic, non-neoplastic constraints usually come upon in orthopedics also in radiology for muscles. The several prognoses of MRI aspects involve strain bruises. Ultrasonography directed steroid vaccination may furnish to less strain. The literature survey of different image processing methods are shown in Table-1

Table 1: Literature Survey of Different Image Processing Methods

METHOD	BENEFITS	DEMERITS	ACCURACY
Triangulation Camera	1.Lofty resolution 2.Lack of essential constraints for dispersions	1.No less than 2 cameras 2.Production cost is high	72%
Flight time period	1.One Camera is sufficient 2.Efficient 3D 3.Low dependability	1. Compact resolution. 2.Complications with reflections	3.66% to 8.96%
Infrared Thermography	1.Swift, viable, exact Alteration 2.A compact potential is necessary	Expensive	80% to 92%

Using the result from above table Momin et al.⁴⁹ evolved the foot pressure sensors along with high susceptibility and compact response time via the MWCNT surfaced cotton fibers which revealed notable features. All the activities performed by the sufferer are gathered using a sensor and observed efficiently and refinement of secure cushion plates is available. The POF-IMU tracking model using a sensor device has been established by Leal-Junior et al.⁵⁰ tendered an investigation of the sensor of POF also IMU implementations. The POF-IMU Sensor model utilizes the angular velocities sustained through the IMU gyroscope to remunerate the physical

phenomenon of the POF sensor. To increase their efficiency, Singla et al.⁵¹ offered a framework for the passive procedure planned to be utilized for lower body rehabilitation appliances of sufferer retrieving from a stroke. It utilized cre software to form the procedure further carried out to MATLAB. The PID controller attains a craved production with compact actuator torques, also function efficiently than the PI controller. Furthermore, Li et al.⁵² presented a flexible and on-line procedure for categorizing lower-limb mobility functioning and also pondered a TMC-HIST with a particular state transition graph to imitate a series of gait and functionalities effectively. Moreover, a flexible on-line procedure attains a high production in functioning categorization.

Li et al.⁵³ pondered a serviceable striding connection, a mutual handle process, and an electric imitation process to furnish solidity response for lower limb paraplegia while wearing a robust exoskeleton, to enumerate for harmed auditory and motorial nerves through hardy fingers. It manages the stride and capable to gather particulars from sensing their functions. Neha-Hooda⁵⁴ shows the combination of EEG, EMG bio fluctuates for the categorization of lower limb motions. The process categorized the five chores with maximal PA. Alterations attains for the handle of robotic models as well as recovery or aid appliances for the sufferer.

CLASSIFICATION OCCURRENCE

The algorithm utilizes digital image processing strategies to lay a simpler process of ankle-foot of gait analysis. Biomechanical classification of particulars is focused at discriminating instinctive separating the usual concepts and morbid ankle-knee sufferers. It is widely categorized into braces strategies. They are statistical as well as ML types. Statistical can be appealed in compact groups and to develop the functions. However, ML is employed in a massive group. This ML is divided into supervised and unsupervised categorizers. By concerning unsupervised classifiers, it splits up into four divisions as follows.

1.1.1. Tree Classifier:

These types of classifiers are usual because it is uncomplicated to decode as well as execute. It has been examined with 5 categorizers. The RT (Regression trees) have appealed towards gait patterns and progressed with 86% of exactness.

1.1.2. Support Vector Machine:

SVM is meant for differentiating processes. It is basically designed for binary classification. Later extended as multiclass classifiers for a large set of data. Each individual's gait patterns have been recorded and it has been processed to furnish an efficient result.

1.1.3. Bayes Classifier:

It is uncomplicated prospective classifiers and a Bayesian network strategy. It is capable of blending with KDE and furnished a better precise value.

Reflective Analysis While Impairment

Simultaneous actions of gait cycles have been recorded, even while the sufferer possesses impairments. The reflective analysis has been carried out to describe the outcomes are mentioned in Figure-4. The phenomenon of gait analysis has been utilized both in young as the well as adults stage sufferers to signifies the process of braces active as well passive process by Slider et al.⁵⁵He presented that usual age-associated variations in the joint while locomotion will not be elevated as a consequence of raised submissive hip joint hardness. The ankle-joint process is vital to concern while utilizing gait study to aid discern adults at complications for impairment. To treat and recover the child those who are suffered from CP via an appliance which is embedded with hardware as well as software. As a result of this drawback, Lerner et al.⁵⁶ exhibited the prospective for an exoskeleton to diminish knee bent throughout the shrink cover from CP lack of essential depletion in self-imposed EMG function.

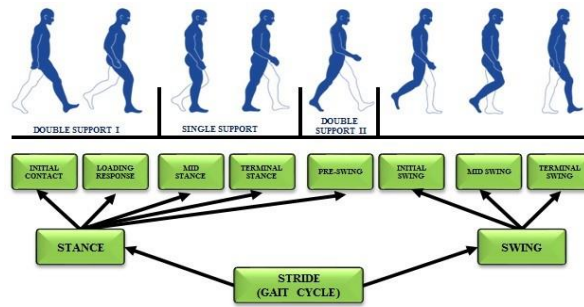


Figure 4: Instance of Gait cycles

Fabrizio Patane et al.⁵⁷ illustrated the assisting device WAKE-up depicted to aid in pediatric sufferers with neurological disorders like CP (Cerebral Palsy). Alteration reveals that the effectiveness of the model in furnishing torques aid in following the self-imposed action. By a little variation in this method Ries et al.⁵⁸ furnished a substantial perception towards variation in assisting device with AFO. The current the tuning technique seems to the absence of vitality, to realize the impacts of every modification done in tuning procedure. So, Nevisipour and Honeycutt⁵⁹ calculated the influence of a semi-rigid AFO. The offsetting striding reaction of healthy man-kinds by diminishing trunk control, compacting length also have lessened the firmness. To overwhelm the disadvantage, Laerke Lindskov et al.⁶⁰ deliberated that ankle-foot orthosis related to variations in the initiation of medial gastrocnemius which will be persistent. The comparative analysis of ankle foot orthosis with different methods is illustrated in Table 2.

Table 2: Comparative Study of Literature Analysis

Author	Year	Report	Method	Implementation
Domenech Novalk ¹³	2014	The research in wearable sensor fusion based robotics with the characters like multimodality, adaptability and performance were discussed, and it also insist on the developers of exoskeleton to check on the sensor fusion.	A wearable sensor fusion based robots for the design of exoskeleton model was used.	In this method raw sensor's data were converted to information according to the action of the wearer by the design engineers.
Nicholas B. Bolus ²	2017	It is competent of braces appealing orthotic resistance as well as observing a substantial set of appropriate objective parameters in a recurrent and authentic way.	An Intermittent Ankle-Foot Orthosis (IAFO)	An IAFO can be utilized to measure an effective outcome of particularly altering the ankle joint hardness.
Matt	20	This is the extension work from the previous	The design of a new	Implemented for people with

he w B ³ 3	1 9	paper of ankle exoskeleton concept by Collins et al. with the consideration of torque assistance regarding form factor work is an extension with the merits of clothing.	unpowered ankle exoskeleton model with low profile, lightweight, less noise and low cost.	different walking speeds, and does not restrict non-sagittal joint motion.
M ari a del Ca rm en Sa nc he zV ill am an an 9	2 0 1 9	Created the set of data sheets that with technical features of the devices, so that the researchers and end-users can have the idea on the recent ideas over existing system.	Mechanical design of wearable exoskeletons deployed in real scenarios	Analysis 52 lower limb's wearable exoskeletons were made with the focus on actuation, structure and interface attachment components.
Fa bri zio Pa tan e ⁵⁷	2 0 1 9	Locomotion of People with cerebral palsy was considered and a module design of new lower limb multi-joint exoskeleton was proposed.	WAKE-up mechanical system is used and also the control architecture and feature extraction are studied.	The method of the WAKE-up design recovered the correct foot landing at the enter point of gait cycle.
Isa o Ab e ³⁷	2 0 1 7	It diminished the load on the tibialis antecedent muscle in the prior posture and oscillates stages.	EEFJ (elastomer-embedded flexible joint)	Fixed a braces EEFJ on handcrafted ankle orthopedic appliance.
Sc ott Pa rd oel 3	2 0 1 9	This study proposes the development and initial testing of a passive ankle exoskeleton intended to provide a plantarflexion torque assist during the push off phase of gait.	The device was integrated with a novel clutch mechanism	A Pneumatic Artificial Muscle acts as a non-linear elastic element to store and release energy during walking.

Karl E. Zelik ¹⁰	2017	In gait analysis ankle and foot power are considered for the interference in science and technology and the assessment are done and prove clinically.	Gait analysis based on foot power and ankle power was made, for the comparison of healthy and the affected person was performed in two cases.	Two case studies were made regarding the ankle and the foot power and the comparison between prostheses and interventions are made. As a result of this study treating entire leg as a rigid body may lead to inappropriate results.
Alvaro Murillo-Herrera ⁴⁶	2019	An idea is categorized as image processing; sensors have aspects that made them effective in various requirements.	A common survey of individuals of gait analysis strategies.	Eventually utilized methodologies like TUG also timed 25-foot.
Joseph M. Laquinto ⁴⁷	2018	Authenticate the production of biplane model for tracking process. It allows a standard and finite motion.	A model hinge on tracking procedure.	Attentiveness towards the ankle and knee kinetics.
Davron Dzhoyn Garfur ⁴¹	2019	WS-based gait uses less, low-power, and low-cost sensors it can enable a periodic re-verification of user identity in personal electronics.	Wearable sensor (WS) based gait consideration.	WS are fixed to the human body to observe the movement of the body parts while walking. The recorded signals are then considered for the individual's recognition purposes.
Meneguzzi	2011	The WS makes a paraplegic patient can walk with the help of	Wearable walking control	A wearable walking controller was

e Li ⁵ 3	7	an exoskeleton. Implemented design was feasible to walk for the paraplegic patients.	interface and an electric stimulation pattern was employed	designed for the voluntarily control of stride when the patient is walking, the electric stimulated simulation were implemented under Feed-back conditions.
Do ng Jin Hy un 30	2 0 1 7	Specifically, an active running gait declare that the proficiency of the robotic leg associated accurately with the human leg, which reveals capability for the proffered scheme in further exoskeletal implementations	HUMA-biomedical model for the lower limb exoskeleton.	A biomedical model for lower limb exoskeleton was implemented for the human leg.
Za ch ar y F. Le rn er ⁵ 6	2 0 1 6	In this method children with cerebral palsy were taken to account. The developed exoskeletons model was based on ankle-foot-orthosis and it also activated the crouch treatment	Wearable sensors based design of exoskeleton.	Excessive knee flexion was reduced during crouch gait from CP. The control techniques for the exoskeleton design were externally done.
J.F . Gu err er o- Ca ste lla no s ²⁹	2 0 1 8	The appraisal is to estimate the viability of the model to aid the gait of a good specialism.	Utilization of AFFO for a typical tracking process in recovery's sake.	The effectiveness of ADRC archetype is authenticate the conceptual investigation.

SUMMARY

This paper offered a review of the models employed in the realization and investigation of striding among methods like image processing; biomechanical details on wearable sensors. Evolution of dissimilar appliances and methods which grant for estimation, performance measures and viable particulars are presented.

1. Many of the study discussed on immediate effect on gait by ankle foot orthoses with considerable increase in speed of walking, length of stride and step, symmetry and posture to swing ratio may cause serious issue.

2. .Random verification is required to find which type of patient are really benefitted out of it to improve the evidence quality.
3. Comparison were made between fixed and hinged AFO and found no results for statistical analysis.
4. The conditioning factor, which might minimize gait function whenever AFO were not in use, was not mentioned in these studies.
5. There was no effective result found for hemiplegic patients, those who can only walk with the aid of AFO.
6. The major drawback in mechanical exoskeleton design is that, if it doesn't perfectly fit the patient, it leads to discomfort and even there is a possibility of discus in muscle.
7. Soft wearable exoskeleton provides maximum comfort to the users with height adjustable calf band, in addition to the control of motion of joint while walking.
8. To modify the normal assisting device, a satisfactory manage method was established and various handle systems were derived.
9. Through NMC-controlled Achilles, it is capable to modify NMC in sequence with ISCI contributors. A compact boost is necessary to upgrade Achilles's aid in assisting device pace. It progressed for an effective refinement thus provides a recovery influence in future investigation.
10. Based on Kinematics AHD as well as SHD strategy is more precise for identifying HS. An exactness of GED upgrades the quality of assisting devices in stroke victims.
11. An ankle-foot orthosis is related to variations in the initiation of medial gastrocnemius which will be persistent. Among the braces orthotic schemes, the AFO with an absolute, compliment footplate associated with the slightest depletion in average muscle movements collected to barefoot while granting an effective muscle functioning in braces muscles.
12. Succeeding studies include elevated samples for better understanding. The foot pressure sensors along with lofty susceptibility and compact response time via the MWCNT surfaced cotton fibers which revealed notable features.
13. All the activities performed by the sufferer are gathered using a sensor and observed efficiently and refinement of secure cushion plates is available. The controller furnishes the appropriate production namely tracking inconsistency while exposed to disruptions occurred. The combination of EEG, EMG bio fluctuates for the categorization of lower limb motions.
14. The wearable interface permits the paraplegic patient to self-control their own action while they walk with the help of an exoskeleton
15. An outcome frame was capable to operate 5 and 3 class collateral. EEG-EMG mechanism furnished with PA of 96.58% and 51.8ms. The process fortuitously categorized the five chores with maximal PA. Alterations attains for the handle of robotic models as well as recovery or aid appliances for the sufferer. An evidencing outcome acquired from the fit state can be widened for handle robotic models.
16. An upcoming survey is required to evaluate effectiveness and adaption in EEG-EMG for reliability analysis with victim inhabitants.

In the previous decades, attentiveness in acquiring depth understanding of assisting device using exoskeleton procedure and activity has elevated enormously. Each strategy differs with compact key aspects. Exploration presented precisely with a massive amount of studies and comprehensive analysis of exploration challenges.

An investigation of the work debated the comprehensive analysis of perceptive challenges and guides the analyst to offer more surveillance in the future. The comforts and performance complications of numerous gait analyses are presented.

REFERENCES

1. Yufeng Zhang, Karen J. Nolan, Damiano Zanotto, Oscillator-based Transparent Control of an Active/Semi-active Ankle-Foot Orthosis, IEEE Robot. Autom. Lett., 2019 Apr;4(2):247-253
2. Nicholas B. Bolus, Caitlin N. Teague, Omer T. Inan, Geza F. Kogler, "Instrumented Ankle-Foot Orthosis: Toward a Clinical Assessment Tool for Patient-Specific Optimization of Orthotic Ankle Stiffness", IEEE ASME Trans Mechatron, 2017 Dec;22(6): 2492-2501.

3. C. B. Sanz-Morere, M. Fantozzi, A. Parri, F. Giovacchini, A. Baldoni, M. Cempini, S. Crea, D. Lefeber, N. Vitiello. A Knee-Ankle-Foot Orthosis to Assist the Sound Limb of Transfemoral Amputees. *IEEE Trans Med Robot Biomech.* 2019 Feb; 1(1):38-48.
4. Ye Ding, Ignacio Galiana, Alan T. Asbeck, Stefano Marco Maria De Rossi, JaehyunBae, ThiagoRibeiroTeles Santos, Vanessa Lara Araujo, Sangjun Lee, Kenneth G. Holt, Conor Walsh. Biomechanical and Physiological Evaluation of Multi-Joint Assistance With Soft Exosuits. *IEEE Trans Neural Syst Rehabil Eng.* 2016 Jan; 25(2):119-130.
5. V.M. Akhil, M. Ashmi, P.K. Rajendrakumar, K.S. Sivanandan. Human Gait Recognition Using Hip, knee and Ankle Joint Ratios. *IRBM.* 2020 June; 41(3):133-140
6. Rachel W. Jackson, Steven H. Collins. An experimental comparison of the relative benefits of work and torque assistance in ankle exoskeletons. *J Appl Physiol.* 2015 Sep; 119(5): 541-557
7. Gong Chen, Peng Qi, Zhao Guo, Haoyong Yu. Gait-Event-Based Synchronization Method for Gait Rehabilitation Robots via a Bio-inspired Adaptive Oscillator. *IEEE Trans Biomed Eng.* 2016 Aug; 64(6):1345-1356.
8. Yunjie Miao, Feng Gao, Dalei Pan. Compound Pendulum Modeling and Resonant Frequency Analysis of the Lower Limbs for the Wearer and Exoskeleton. *J Bionic Eng.* 2015 July; 12(3):372-381.
9. Maria del Carmen Sanchez-Villamanan, Jose Gonzalez-Vargas, Diego Torricelli, Juan C. Moreno, Jose L. Pons. Compliant lower limb exoskeletons: a comprehensive review on mechanical design principles. *Journal of Neuro Engineering and Rehabilitation.* 2019 May; 16(1).
10. Karl E. Zelik, Eric C. Honert. Ankle and foot power in gait analysis: Implications for science, technology and clinical assessment. *Journal of Biomechanics.* 2018 June; 75:1-12.
gait based on motion analysis. *Medical Engineering & Physics.* 2019 Jan; 63:33-41.
11. Gong Chen, Peng Qi, Zhao Guo, Haoyong Yu. Mechanical design and evaluation of a compact portable knee-ankle-foot robot for gait rehabilitation. *Mechanism and Machine Theory.* 2016 Sep; 103:51-64.
12. Stacey R. Zhao, J. Timothy Bryant, Qingguo Li. Deformable link segment analysis for prosthetic foot-ankle components: Kinematics. *J Biomechanics.* 2020 Jan; 99:109548
13. Domen Novak, Robert Riener. A Survey of sensor fusion methods in wearable robotics. *Robotics and Autonomous Systems.* 2015 Nov; 73:155-170.
14. Xiangyang Wang, Sheng Guo, Haibo Qu, Majun Song. Design of a Purely Mechanical Sensor-Controller Integrated System for Walking Assistance on Ankle-Foot Exoskeleton. *Sensors (Basel).* 2019 Jul; 19(14):3196.
15. Fangli Yu, Jianbin Zheng, Lie Yu, Rui Zhang, Hailin He, Zhenbo Zhu, Yuanpeng Zhang. Adjustable Method for Real-Time Gait Pattern Detection Based on Ground Reaction Forces Using Force Sensitive Resistors and Statistical Analysis of Constant False Alarm Rate. *Sensors (Basel).* 2018 Nov; 18(11):3764.
16. Luke M. Mooney, Hugh M. Herr. Biomechanical walking mechanism underlying in metabolic reduction caused by an autonomous exoskeleton. *J Neuro Eng Rehabil.* 2016 Jan; 13(4).
17. Juri Taborri, Eduardo Palermo, Stefano Rossi, Paolo Cappa. Gait Partitioning Methods: A Systematic Review. *Sensors (Basel).* 2016 Jan; 16(1):66.
18. Jing Tang, Jianbin Zheng, Yang Wang, Lie Yu, Enqi Zhan, Qiuzhi Song. Self-Tuning Threshold Method for Real-Time Gait Phase Detection Based on Ground Contact Forces Using FSRs. *Sensors (Basel).* 2018 Feb; 18(2):481.
19. Yi Long, Zhijiang Du, Chaofeng Chen, Weidong Wang, Long He, Xiwang Mao, Guoqiang Xu, Guangyu Zhao, Xiaoqi Li, Wei Dong. Development and Analysis of an Electrically Actuated Lower Extremity Assistive Exoskeleton. *Journal of Bionic Engineering.* 2017 July; 14(2):272-283.
20. Johnny D. Farah, Natalie Baddour, Edward D. Lemaire. Design, development, and evaluation of a local sensor-based gait phase recognition system using a logistic model decision tree for orthosis-control. *J Neuroeng Rehabil Eng.* 2019 Feb; 16(1):22-44.
21. Hwan Choi, Keshia M. Peters, Michael B. MacConnell, Katie K. Ly, Eric S. Eckert, Katherine M. Steele. Impact of ankle foot orthosis stiffness on Achilles tendon and gastrocnemius function during unimpaired gait. *Journal of Biomechanics.* 2017 Nov; 64:145-152.

22. Victor Arnez-Paniagua, Hala Rifai, Samer Mohammed, Yacine Amirat. Adaptive Control of an Actuated Ankle Foot Orthosis for Foot-Drop Correction. *IFAC-Papers On Line*. 2017 July;50(1):1384-1389.
23. Fatai Sado, Hwa Jen Yap, Raja Ariffin Raja Ghazilla, Norhafizan Ahmad. Exoskeleton robot control for synchronous walking assistance in repetitive manual handling works based on dual unscented Kalman filter. *PLOS ONE*. 2018 July;13(7).
24. Mario C. Faustini, Richard R. Neptune, Richard H. Crawford, Steven J. Stanhope. Manufacture of Passive Dynamic Ankle-Foot Orthoses Using Selective Laser Sintering. *IEEE Transactions on Biomedical Engineering*. 2008 Feb;55(2):784-90.
25. Takahiro Oba, Hideki Kadone, Modar Hassan, Kenji Suzuki. Robotic Ankle-Foot Orthosis With a Variable Viscosity Link Using MR Fluid. *IEEE/ASME Transactions on Mechatronics*. 2019 April;24(2): 495-504.
26. Starr E. Brown, Elizabeth Russell Esposito, Jason M. Wilken. The effect of ankle foot orthosis alignment on walking in individuals treated for traumatic lower extremity injuries. *J Biomechanics*. 2017 Aug;61.
27. Margret A. French, Corey Koller, Elisa S. Arch. Comparison of three kinematic gait event detection methods during over ground and treadmill walking for individuals post stroke. *J Biomechanics*. 2020 Jan;99:109481.
28. Nils Eckardt, Armin Kibele. Automatic Identification of gait events during walking on uneven surfaces. *Gait & Posture*. 2017 Feb;52:83-86.
29. J.F. Guerrero-Castellanos, H. Rifai, V. Arnez-Paniagua, J. Liarez-Flores, L. Saynes-Torres, S. Mohammed. Robust Active Disturbance Rejection Control via control Lyapunov functions: Application to Actuated-Ankle-Foot-Orthosis. *Control Engineering Practice*. 2018 Nov;80:49-60.
30. Dong Jin Hyun, Hyunseok Park, Taejun Ha, Sangin Park, Kyungmo Jung. Biomechanical design of an agile, electricity-powered lower-limb exoskeleton for weight-bearing assistance. *Robotics and Autonomous Systems*. 2017 Sep;95:181-195.
31. Scott Pardoel, Marc Doumit. Development and testing of a passive ankle exoskeleton. *Biocybernetics and Biomedical Engineering*. 2019 Sep;39(3):902-913.
32. Kashif I.K. Shrewani, Neelesh Kumar, Ahmed Chemori, Munna Khan, Samer Mohammed. RISE-based adaptive control for EICoSI exoskeleton to assist knee joint mobility. *Robotics and Autonomous Systems*, 2020 Feb;124:103354.
33. Matthew B. Yandell, Joshua R. Tacca, Karl E. Zelik. Design of a Low Profile, Unpowered Ankle Exoskeleton That Fits Under Clothes: Overcoming Practical Barriers to Widespread Societal Adoption. *IEEE Trans Neural Syst Rehabil Eng*. 2019 Apr;27(4):712-723.
34. Valentina Agostini, Gabriella Balestra, and Marco Knaflitz. Segmentation and Classification of Gait Cycles. *IEEE Trans Neural Syst and Rehabil Eng*. 2014 Jan;22(5):946-952.
35. Ming Liu, Fan Zhang, He Huang. An Adaptive Classification Strategy for Reliable Locomotion Mode Recognition. *Sensors (Basel)*. 2017 Sep;17(9):2020.
36. Houssein Lamine, Med Amine Laribi, Sami Bennour, Lotfi Romdhane, Said Zeghloul. Design Study of a Cable-based Gait Training Machine. *J Bionic Eng*. 2017 April;14(2): 232-244.
37. Isao Abe, Kohei Ishiya, Taiki Oshimoto, Takehito Kikuchi, Sosuke Tanida, Takashi Yasuda. Ankle-foot orthosis using elastomer-embedded flexible joint. 2017 39th Annual International Conference of the IEEE Engineering in Medicine and Biology Society (EMBC), 2017 Sep.
38. F. Tamburella, N. L. Tagliamonte, I. Pisotta, M. Masciullo, M. Arquilla, E. H. F. van Asseldonk. Neuromuscular Controller Embedded in a Powered Ankle Exoskeleton: Effects on Gait, Clinical Features and Subjective Perspective of Incomplete Spinal Cord Injured Subjects. *IEEE Trans Neural Syst Rehabil Eng*. 2020 May;28(5):1157-1167.
39. Bikash Roy, Subhasis Bhaumik, Jayanta Kumar Chakraborty. Detection of Gait Characteristic Using Image Processing Technique. *Trends Biomater. Arif. Organs*. 2004;17(2):503-510.
40. Ramanpreet Singh, Himanshu Chaudhary, Amit K. Singh. A novel gait-based synthesis procedure for the design of 4-bar exoskeleton with natural trajectories. *Journal of Orthopaedic Translation*. 2018 Jan;12:6-15.
41. Davrondzhon Gafurov, Einar Snekkenes. Gait Recognition Using Wearable Motion Recording Sensors. *Journal on Advances in Signal Processing (EURASIP)*. 2009 June:415817.

42. Mario Nieto-Hidalgo, Francisco Javier Ferrandez-Pastor, Rafael J. Valdiviesco-Sarabia, Jeronimo Mora-Pascual, Juan Manuel Garcia-Chamizo. A vision based proposal for classification of normal and abnormal gait using RGB camera. *Journal of Biomedical Informatics*. 2016 Oct;63:82-89.
43. S. Park, S. Lee, J Yoon, SW Chae. Finite element analysis of knee and ankle joint during walking. *Journal of Biomedical Informatics*. 2016 Oct;63:82-89.
44. Lei Yan, Tao zhen, Jian-Lei Kong, Lian-Ming Wang, Xiao-Lei Zhou. Walking Gait Phase Detection Based on Acceleration Signals Using Voting-Weighted Integrated Neural Network. *Dynamical Analysis of Biological Systems*. 2020 Jan:1-14.
45. Mario Nieto-Hidalgo, Francisco Javier Ferrandez-Pastor, Rafael J. Valdiviesco-Sarabia, Jeronimo Mora-Pascual, Juan Manuel Garcia-Chamizo. Gait Analysis Using Computer Vision Based on Cloud Platform and Mobile Device. *Ambient Assisted Living and Ambient Intelligence for Health*. 2018 Jan.
46. Alvaro Muro-de-la-Herran, Begonya Garcia-Zapirian, Amaia Mendez-Zorrilla. Gait Analysis Methods: An Overview of Wearable and Non-Wearable Systems, Highlighting Clinical Applications. *Sensors (Basel)*. 2019 Feb;14(2):3362-3394.
47. Joseph M. Iaquinto, Matthew W. Kindig, David R. Haynor, QuocBao Vu, Nathan Pepin, Richard Tsai, Bruce J. Sangeorzan, William R. Ledoux. Model-based tracking of the bones of the foot: A biplane fluoroscopy validation study. *Computers in Biology & Medicine*. 2018 Jan;92:118-127.
48. Sinan Al-Qassab, Alun Davies. Imaging of the foot and ankle. *Gait & Posture*. 2020 Feb;38(2):100-107.
49. Md. Abdul Momin, Mohammad Jellur Rahman, Tetsu Mieno. Foot pressure sensor system made from MWCNT coated cotton fibers to monitor human activities. *Surface & Coatings Technology*. 2020 July;394:125749.
50. Arnaldo G. Leal-Junior, Lara Vargas-Valencia, Wilian M. dos Santos, Felipe B. A. Schneider, Adriano A.G. Siqueira, Maria Jose Pontes, Anselmo Frizzera. POF-IMU sensor system: A fusion between inertial measurement units and POF sensors for low-cost and highly reliable systems. *Optical Fiber Technology*. 2018 July;43:82-89.
51. Ashish Singla, Gurminder Singh, Gurvinder Singh Virk. Matlab/simMechanics based control of four bar passive lower body mechanism for rehabilitation. *Perspectives in Science*. 2016 Sep;8:351-354.
52. Haoyu Li, Stephane Derrode, Wojciech Pieczynski. An adaptive and on-line IMU-based locomotion activity classification method using a triplet Markov model. *Neurocomputing*. 2019 Oct;362:94-105.
53. Mengze Li, Zhaofan Yuan, Xufeng Wang, Yasuhisa Hasegawa. Electric Stimulation and cooperative control for paraplegic patient wearing an exoskeleton. *Robotics and Autonomous Systems*. 2017 Dec;98:204-212.
54. Neha Hooda, Ratan Das, Neelesh Kumar. Fusion of EEG and EMG signals for classification of unilateral foot movements. *Biomedical Signal Processing and Control*. 2020 July;60:101990.
55. Amy Silder, Bryan Heiderscheit, Darryl G. Thelen. Active and passive contributions to joint kinetics during walking in older adults. *J Biomech*. 2008 Apr ;41(7):1520-1527.
56. Zachary F. Lerner, Diane L. Damiano, Hyung-Soon Park, Andrew J. Gravunder, Thomas C. Bulea. A Robotic Exoskeleton for Treatment of Crouch Gait in Children with Cerebral Palsy: Design and Initial Application. *IEEE Trans Neural Syst Rehabil Eng*. 2017 Jun; 25(6): 650-659.
57. Fabrizio Patane, Stefano Rossi, Fausto Del Sette, Juri Taborri, Cappa. Wake-up Exoskeleton to assist children with Cerebral Palsy: design and preliminary evaluation in level walking. *IEEE Trans Neural Syst Rehabil Eng*. 2017 Jul;25(7):906-916.
58. AJ Ries, TF Novacheck, MH Schwartz. The Effectiveness of Ankle-Foot Orthoses on Improving the Gait of Children with Diplegic Cerebral Palsy: A Multiple Outcome Analysis. *PM & R*. 2015 Sep;7(9):922-929.
59. Masood Nevisipour, Claire F. Honeycutt. The impact of ankle-foot-orthosis (AFO) use on the compensatory stepping response required to avoid a fall during trip-like perturbations in young adults: Implications for AFO prescription and design. *J Biomechanics*. 2020 April;103:10703.

60.LaerkeLindskov, Ann-Britt Huse, Marie Johansson, Stale Nygard. Muscle activity in children with spastic unilateral cerebral palsy when walking with ankle-foot orthoses: an explorative study. *Gate & Posture*.2020 July;8:31-36.